





Congratulations on your rental of the VascuTherm3. You are well on your way to a speedy recovery. Please consult the following instructions or our step by step instructional video @ www.peakmedicalgroup.com before using your device. If at the end of these instructions you still require assistance, you can call our toll free helpline (phone #'s on the last page). During winter months, please ensure the device is room temperature before use.

1. Unpack your system. Be sure to **keep the packing material and box** as this will be used to send the device back to Peak Medical Group. You will notice that a **waybill for Purolator** (label with our address) has been included in the box. This waybill will be attached to the box once repacked to ensure no charge return shipping for the device. Inside the box you will find:

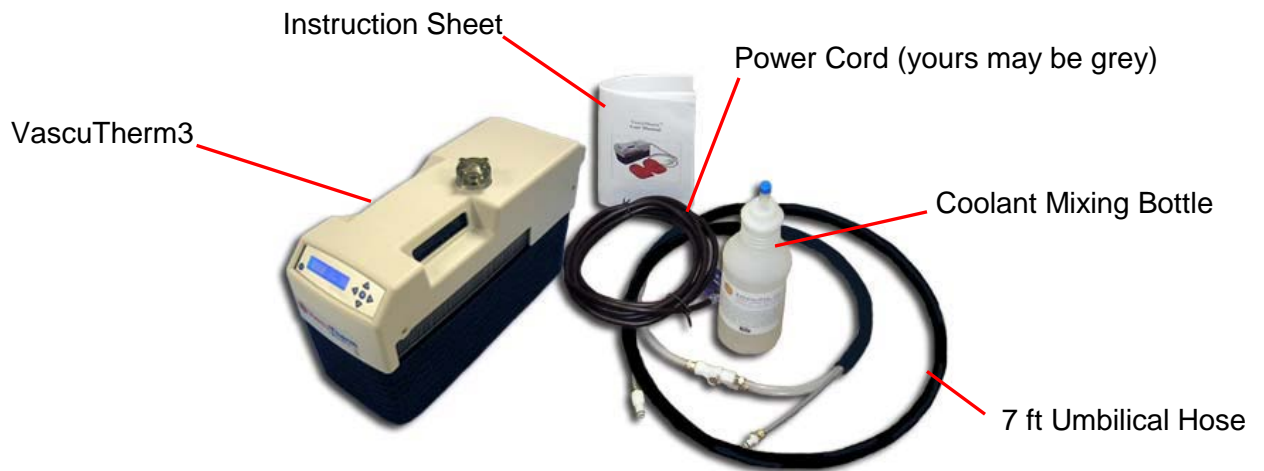

Other materials in box: Purolator waybill for return shipment. **You will also find your therapeutic wrap or wraps.**


2. Unscrew the cap on the top of the device and pour in the coolant mixture until the coolant level is above the halfway mark on the viewing window. The viewing window is located on the side of the device. You will not need to use the entire bottle of fluid and please be sure to replace the cap.

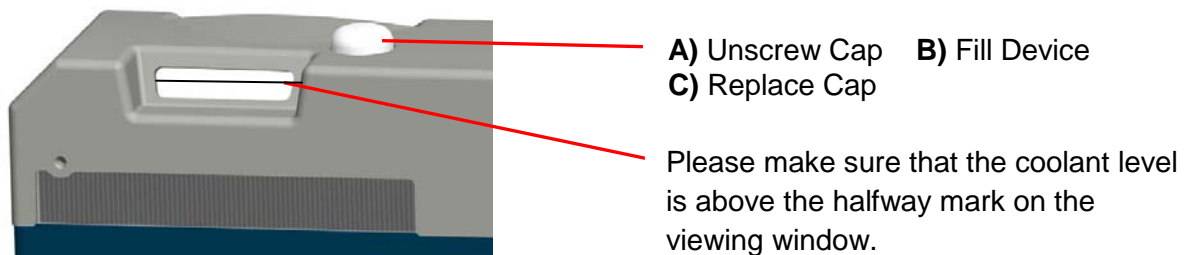

** Coolant level may drop within the first few minutes of use. If coolant level can be seen lower than halfway down the window once therapy is started, more coolant should be added. There is a warning on the device if coolant level becomes too low reminding you to add more.


3. Attach the grey power cord to the back of the VascuTherm3. Plug the other end into an outlet within 10 ft of where you would like to enjoy your therapy.
4. As pictured below attach the “Male Ends” of the 7ft black umbilical cord to the top left corner of the back of the Vascutherm3. Push the ends in until you hear a clicking sound.

Attach 7 ft umbilical cord. Push ends in until they ‘click’. There is no wrong way to do this.

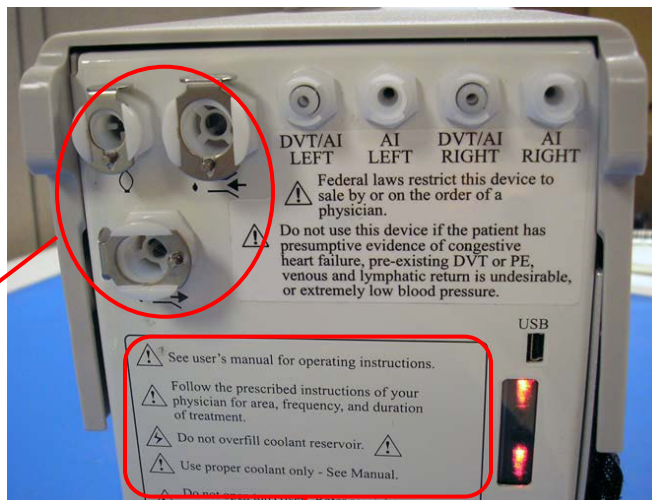

Grey power cord attaches just below text box pictured

5. **Skip this step if NO DVT therapy has been prescribed.** If you have been prescribed DVT therapy, you must first open the bag that contains your DVT wraps. The front of the bag will say ‘DVT calf wrap set OR DVT foot wrap set’. Once opened, connect the wrap by pushing the blue ends of the hose into the slots labelled for your therapy (these slots are located on the top right corner of the back of the Vascutherm3) There will always be 2 DVT wraps per bag. You may only need one depending on your therapy. If so, disregard one of the wraps.

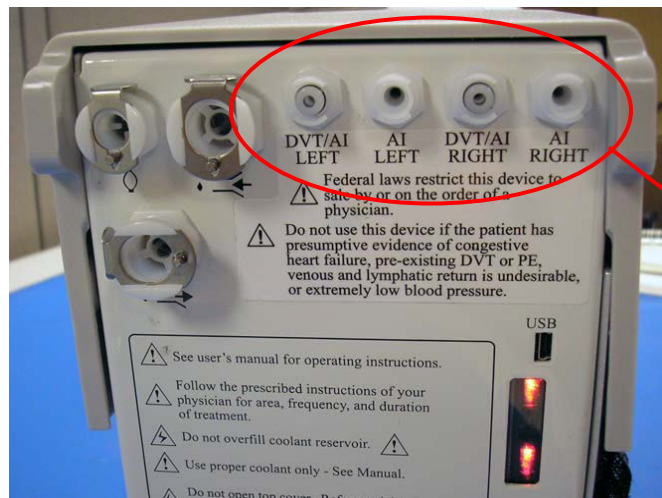


Insert DVT fitting into opening labelled for your therapy. **You have been prescribed**

6. Now you are ready to attach your therapeutic wrap to the other end of the black umbilical cord. Open the bag that contains your therapeutic wrap and **remove the red coloured caps** on the end of the hoses. Connect these ends to the open end of your 7ft umbilical cord. You will hear a ‘clicking’ sound when connected properly. For instructions on how to place the wrap on your body, there is an instruction sheet included in the bag that contained the wrap.

You are now ready to start your therapy!! The VascuTherm3 has been pre-programmed for your therapy under the recommendations of a medical professional.

7. Turn on your device by using the red switch located on the back of the VascuTherm3 just above where the grey power cord is attached. You will see the following screens on the front of the device.

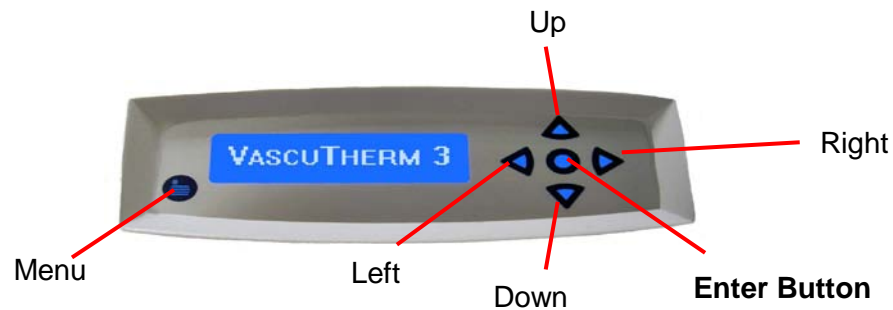

This is the next screen that you will see.




8. Be sure to have your **wrap/wraps in place** before starting your therapy. Follow the instructions on how to place the wrap on your body provided in the bag that contains your wrap. Be sure that the hoses connected to the wrap are facing downwards and that the 'bubble side' of the wrap is against your body. The Velcro straps for the wraps attach to the 'fuzzy side' of the wrap. **It is not necessary to place the wrap on your skin, you can receive therapy through your clothing or bandages if you prefer.**
9. Your therapy has been pre-programmed by Peak Medical Group. You will want to **resume** the **therapy** that has been programmed for you. You must simply press the enter button (pictured above) to start your therapy. The device will cycle through its therapy session until you decide to stop therapy.
10. To stop your therapy, press the enter button (pictured above) and you will see a screen that is very similar to the start up screen except for where RESUME THERAPY once was there is now **STOP THERAPY**. Simply press the enter button again to stop your therapy. **You will be pressing the enter button a total of two times to stop your therapy.** Once your therapy is stopped you can remove your wraps and turn off the machine by using the switch on the back of the device. At any time you can resume your therapy by following steps 6 through 8.

YOU HAVE BEEN PRESCRIBED _____ HOUR(S) OF THERAPY PER DAY.

The device will remember your treatment program in between sessions. The device also records the amount of time you have spent on your therapy.

11. At the end of your treatment period (the number of days that you have used the device) Peak Medical Group will have arranged for the pick-up of your machine. Please remove all cables by pressing the silver tabs where they connect to the Vascutherm3 and where they connect to your wrap. For DVT therapy simply remove the cables by pulling gently towards you. **Please ensure that all liquid has been emptied from the device before repacking** (fluid left in device may cause damage during shipment).

Empty fluid into sink,
replace cap once
finished.

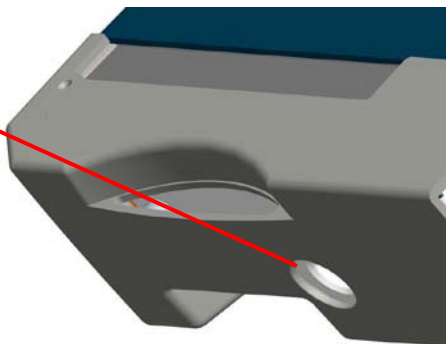

12. **Carefully repack the device** as you received it with the box and packing foam provided. Include all of the materials that you found inside the box (please refer to checklist below). It is **NOT** necessary to send back your therapeutic wraps as these are intended for single patient use.
13. Remove the existing Purolator way bill from the outside of the box and replace it with the new one provided to you.

CHECKLIST FOR RETURN OF DEVICE:

- ① VASCUTHERM 3 ② POWER CORD ③ COOLANT BOTTLE ④ 7FT UMBILICAL CORD

**ANY MISSING OR DAMAGED PIECES MAY RESULT IN A CHARGE TO THE PATIENT.

YOUR DEVICE HAS BEEN SCHEDULED FOR PICK-UP ON: _____.

IF YOU ARE UNABLE TO BE AT HOME FOR THE DELIVERY DRIVER, PLEASE CONTACT PEAK MEDICAL GROUP TO ARRANGE ALTERNATE PLANS @ 1-800-757-4635. MISSED PICK-UP MAY RESULT IN FURTHER RENTAL CHARGES.

TOLL FREE HELPLINE

Monday to Friday/ 8am -5pm/Central Time

1-800-242-3232 or 1-800-757-4635

Evenings and Weekends

Call 1-800-242-3232 and choose the option for Technical Support, this will connect you to a live individual.